
## Face shield N2 Assembly instructions



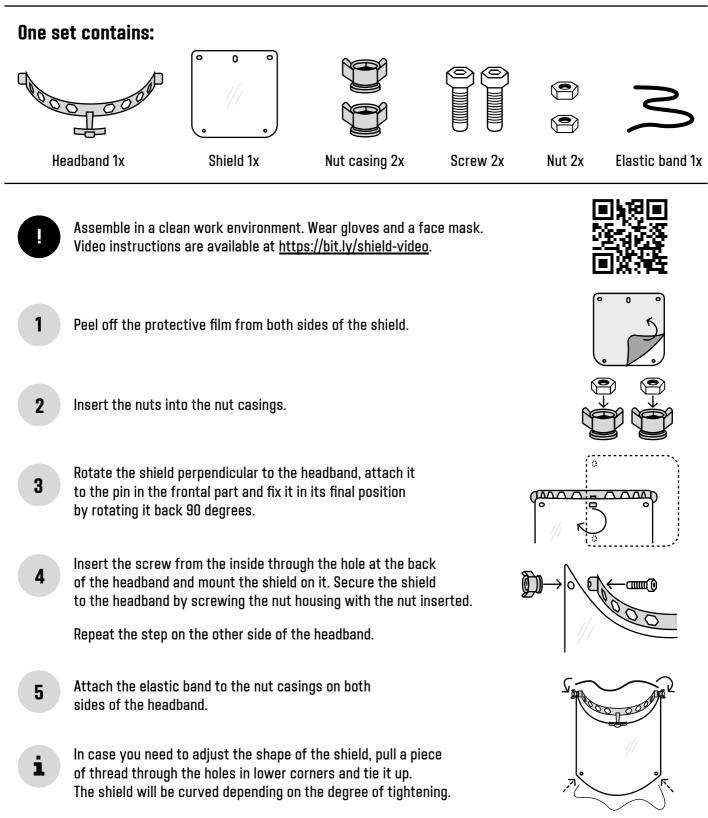

## Maintenance:

Use common disinfectants such as ethanol for disinfecting the face shield. The shield can be sterilized in systems using low-temperature hydrogen peroxide plasma (STERRAD). Do not expose the shield to temperatures exceeding 60 °C / 140 °F.

Manufactured by Y Soft Corporation. Designed by Tiskne celé Česko. Funded by Y Soft Corporation with contribution of American Chamber of Commerce, Livesport company and RSJ financial group. Not for sale.



